

MediSense[®]

Precision Xtra[™]

Advanced Diabetes Management System

User's Guide



a
ABBOTT

For *in vitro* diagnostic use.

Table of Contents

	Welcome	1
1	Important Things to Know about Your Precision Xtra Advanced Diabetes Management System	3
	Intended Use	3
	How Your Precision Xtra Advanced Diabetes Management System Works	4
	Precision Xtra Kit Contents	5
	Getting to Know Your Monitor's Features	6
2	Setting Up Your Precision Xtra Monitor	9
	Buttons to Use	9
	Setup Options	9
	How to Set the Beeper, Date, Time, & View Measurement Units	11
	Set Beeper	11
	Set Time	13
	Set Date	15
	Set Time Format	18
	Set Date Format	19
	Blood Glucose Measurement Units	20
3	Calibrating Your Precision Xtra Monitor	22
	Why Calibrate Your Monitor?	22
	When to Calibrate Your Monitor	22
	What You Will Need	23
	How to Calibrate Your Monitor	23
	How to Recall the LOT Number or Calibration CODE	28
4	Monitoring Your Blood Glucose	30
	What You Will Need	30
	Important Information about Monitoring Your Blood Glucose	30
	How to Monitor Your Blood Glucose	31
	Understanding Your Result	39
5	Monitoring Your Blood β-Ketone	43
	What You Will Need	43
	Important Information about Monitoring Your Blood β -Ketone	44
	How to Monitor Your Blood β -Ketone	45
	Understanding Your Result	52

6	Doing A Control Solution Test	55
	Why Do A Control Solution Test?	55
	When Is Doing A Control Solution Test Recommended?	55
	Important Information about Control Solution Testing	55
	What You Will Need	57
	How to Do Control Solution Testing	57
	Understanding Your Result	64
7	Reviewing & Using Your Results	65
	What Can Your Monitor Show You?	65
	How to See Results in Memory	66
	How to See Averages	69
	Transferring Your Results to A Computer	71
8	Understanding & Troubleshooting Error Messages	72
	What An Error Message Means & What You Need to Do	72
9	Your Monitor's Specifications & Limitations	77
	Important Information about Using Blood Samples from the Forearm, Upper Arm, or Base of the Thumb	80
10	Caring For Your Monitor	82
	Cleaning Your Monitor	82
	Replacing Your Monitor's Battery	83
11	Support, Guarantee & Limited Warranty	87
	References	89

Welcome

Thank you for choosing the Precision Xtra™ Advanced Diabetes Management System.

Important steps for using the System are inside this guide. Please read it carefully.

Your new Precision Xtra Advanced Diabetes Management System is an important tool that can help you better manage your diabetes. The System measures both blood glucose (sugar) and blood β -Ketone. Blood glucose and blood β -Ketone results can help you understand your diabetes and what happens with:

- Food
- Exercise
- Stress and illness
- Diabetes medications

Always monitor your blood glucose and blood β -Ketone according to your healthcare professional's recommendations.

In the United States, call Customer Care at 1-800-527-3339 with any questions you may have about the Precision Xtra Advanced Diabetes Management System. We are available 24 hours a day, 365 days a year. If you cannot reach Customer Care, contact your healthcare professional.

Outside the United States, please contact your local Abbott Laboratories, Abbott Diabetes Care office or distributor.

Please read the following items before using your Precision Xtra Advanced Diabetes Management System:

- [User guide](#)
- [Blood glucose test strip instructions for use](#)
- [Blood \$\beta\$ -Ketone test strip instructions for use](#)
- [Lancing device instructions for use and other information](#)
- [Warranty card](#)

IMPORTANT:

Any user guide text shown in a shaded box like this one is important information. Please pay special attention to these boxes.

Important Things to Know about Your Precision Xtra Advanced Diabetes Management System

Questions? Call
Customer Care:
1-800-527-3339

Important
Information

► Intended Use

Your Precision Xtra System:

- Is indicated for home (lay user) or professional use in the management of Patients with diabetes.
- Is for use outside the body (*in vitro* diagnostic use).
- Is for monitoring glucose in fresh whole blood (for example, from the fingertip).
- Is for monitoring β -Ketone in fresh whole blood from the fingertip.
- Measures β -hydroxybutyrate (β -Ketone), the most important of the three ketone bodies circulating in the bloodstream.
- Is for use with Precision Xtra™ or Precision™ POC Blood Glucose Test Strips and Precision Xtra™ Blood β -Ketone Test Strips.



- Precision Xtra™ and Precision™ POC Blood Glucose Test Strips are different. Please refer to your test strip instructions for use for important information about sample types that may be used with these test strips.
- Precision™ POC Blood Glucose Test Strips are for use by healthcare professionals only.



Potential Infection Risk:

Healthcare professionals performing blood tests with this system on multiple patients must always wear gloves and should follow the infection control policies and procedures approved by their facility.

► How Your Precision Xtra Advanced Diabetes Management System Works

When you insert a test strip into your monitor, the Apply Blood message shows on your monitor's display window. When a blood sample or control solution sample is applied to the test strip, the glucose or β -Ketone reacts with the chemicals on the test strip. This reaction produces a small electrical current that is measured. The result shows on your monitor's display window.

► Precision Xtra Kit Contents

Precision Xtra Monitor

Precision Xtra User's Guide

– Contains system information and directions.

Carrying Case

– Use this to store and carry your monitor and other monitoring supplies.

Your kit may also contain:

Precision Xtra Quick Reference Guide

– Gives the basic steps to calibrate your monitor and check your blood glucose.

Logbook

– Use this to record your test results, activities, and medications.

Precision Friends for Life Card

– Please fill this out and return to the address provided to activate your warranty. Filling out this card helps to ensure that you receive any updates regarding your Precision Xtra monitor.

Lancing Device, Lancets, Instructions for Use and Other Information

Blood Glucose Test Strips and Instructions for Use


Items not included:
 MediSense Control Solutions
 Blood β -Ketone Test Strips
 and Instructions for Use
 Data Management System

▶ Getting to Know Your Monitor's Features

Display Window

This shows:

- Blood glucose and blood β -Ketone results
- Glucose LOT numbers and β -Ketone calibration CODEs
- Previous test results and error messages
- Blood glucose averages

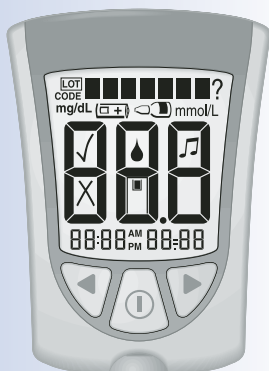


Display Check

IMPORTANT:

Each time you turn your monitor on, a full display shows. This is called a Display Check. Look at the Display Check each time it appears on your monitor's display window, especially before you check your blood glucose or blood β -Ketone. The Display Check shows on the display window briefly.


Do not use the monitor if the monitor Display Check does not exactly match the picture here (for example, if you see a "3" instead of an "8"). The monitor may show an incorrect result when you use it. Please call Customer Care for assistance.

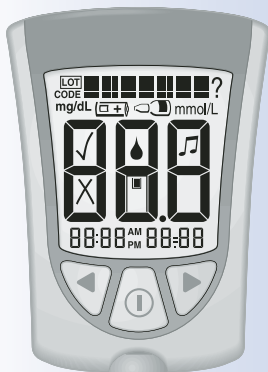

Strip Port

This is where you insert:

- A blood glucose test strip
- A blood β -Ketone test strip
- A glucose calibrator
- A ketone calibrator
- Data cable (not included) for uploading results to a computer



Mode Button

Use this button to:

- Turn monitor ON and OFF
- Access monitor setup options
- Access and save monitor settings
- Access previous results and averages

▶ Forward Button

◀ Back Button

Use these buttons to:

- Review and select monitor settings
- Review results and averages

Backlight Button


Use this button to:

- Turn backlight ON and OFF

Battery Compartment

This is where the battery is installed.

- If your monitor does not turn on, check that your battery is installed properly.
- For new battery installation, see Chapter 10.



Setting Up Your Precision Xtra Monitor

Questions? Call
Customer Care:
1-800-527-3339

▶ Buttons to Use

- ① Mode Button
- ▶ Forward Button
- ◀ Back Button



▶ Setup Options

Set Beeper

If the beeper is set ON, it will beep when:

- The calibrator is fully inserted
- The test countdown starts
- The test countdown finishes

Set Time, Set Date

Important: Set the correct time and date before you use the monitor for the first time. This will help you keep records of when you monitor and will help you and your healthcare professional make informed decisions about your care.

You must set the time and date to review averages.

You may need to re-set the time and date:

- After you replace the battery.
- When you travel between time zones or when the time zone you are in changes.

In "Set Date", you set the year, month, and day.

Set Time Format

In "Set Time Format", you choose how the time shows on the monitor's display window.

Set Date Format

In "Set Date Format", you choose how the month and day show on the monitor's display window.

Measurement Units

Blood glucose measurement units are factory-set in mg/dL or mmol/L.


Blood B-Ketone measurement units are in mmol/L only.


► How to Set the Beeper, Date, Time, & View Measurement Units

To begin, pull the battery tab out. Your monitor should be turned OFF.

Before you start, please

note: "Press and Hold" means that you press the button in for at least 2 seconds. "Press and Release" means that you press the button and let it go quickly.


Press and Hold the  button to turn the monitor off and save your settings at any time. The monitor automatically turns off after 30 seconds of no action.

If you like the setting that you see on your monitor and do not want to change it, Press and Release the  button to move to the next setup option.

Set Beeper

The ✓ means the beeper is ON.


The X means the beeper is OFF.

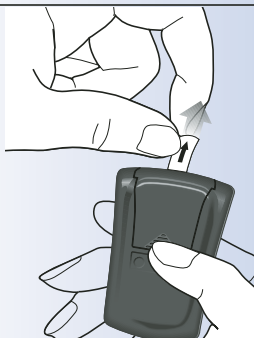


Beeper ON




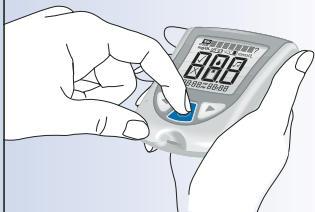

Beeper OFF




1 To turn your monitor ON, Press and Hold the  button.

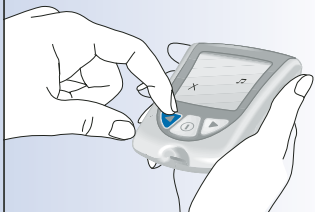The beeper ON message shows on the display window. The musical notes flash on and off, and the monitor beeps.



2 To change the beeper setting, Press and Release the  button or the  button once.



3 Press and Release the  button to save the beeper setting and to move to Set Time (Hour).


Set Time

Hour:


The Hour flashes on and off.



- 1 Press and Release the ► button to move the hour forward.

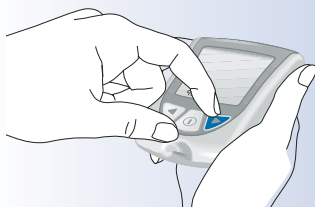

- 2 If you go past the correct hour, Press and Release the ◀ button to move the hour back.

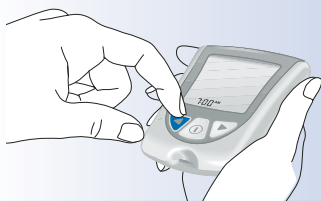


- 3 Press and Release the ⓘ button to save the hour and to move to Set Minutes.






Minutes:

The Minutes flash on and off.

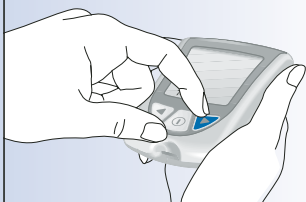

1 Press and Release the ► button to move the minutes forward.

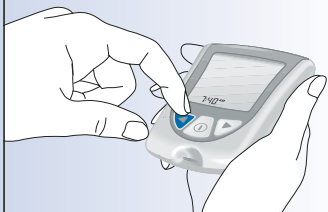

2 If you go past the correct minute, Press and Release the ◀ button to move the minutes back.



3 Press and Release the ⓘ button to save the minutes and to move to Set Date.


Set Date

Year:


The Year flashes on and off.




- 1 Press and Release the ► button to move the year forward.

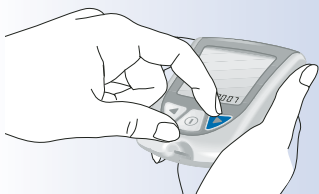

- 2 If you go past the correct year, Press and Release the ◀ button to move the year back.

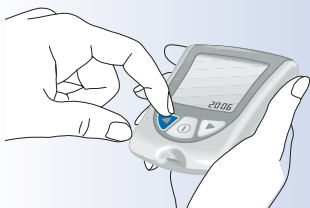


- 3 Press and Release the ⓘ button to save the year and to move to Set Month.

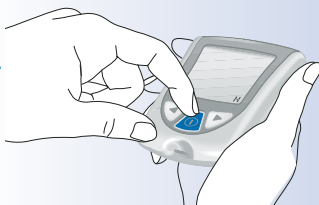




Month:


The Month flashes on and off.



1 Press and Release the ► button to move the month forward.



2 If you go past the correct month, Press and Release the ◀ button to move the month back.




3 Press and Release the ⓘ button to save the month and to move to Set Day.

Day:


The Day flashes on and off.




- 1 Press and Release the ► button to move the day forward.

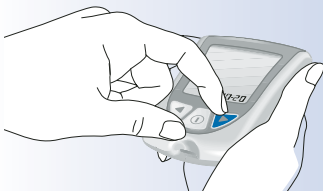


- 2 If you go past the correct day, Press and Release the ◀ button to move the day back.

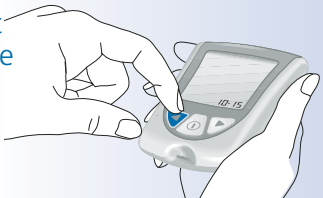

- 3 Press and Release the ⓘ button to save the day and to move to Set Time Format.

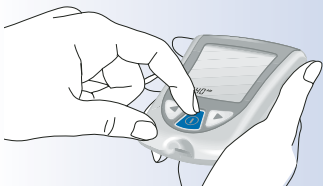

Choice #1

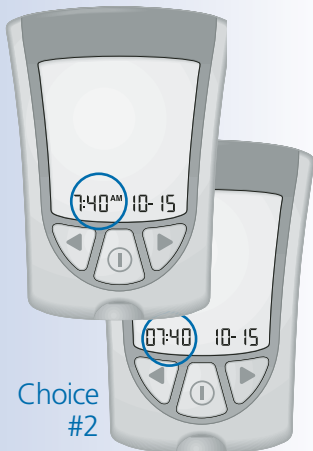


Choice #2

Set Time Format


You have two choices:

Choice #1: For the 12-hour format, AM or PM shows.

Choice #2: For the 24-hour format, AM or PM does not show.



- 1 To change the Time Format, Press and Release the ◀ button or the ▶ button once.

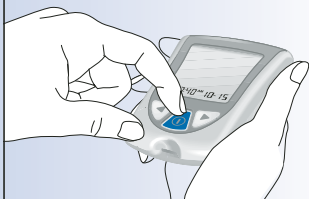

- 2 Press and Release the ⓘ button to save the Time Format and to move to Set Date Format.

Set Date Format

You have two choices:

Choice #1: For the month-day format, "■" shows with the date.


Example:

"May 25" shows as "5-25".


Choice #2: For the day.month format, "●" shows with the date.

Example:


"25 May" shows as "25.5".

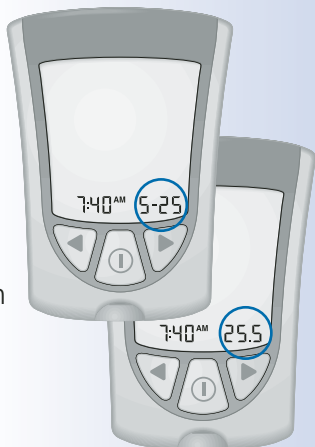


- 1 To change the Date Format, Press and Release the ◀ button or the ▶ button once.



- 2 Press and Release the ⓘ button to save the Date Format and to move to Measurement Units.




Blood Glucose Measurement Units

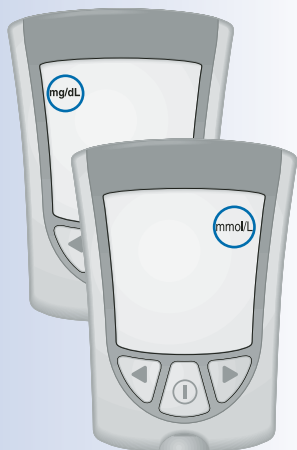


Consult your healthcare professional if you have any questions about blood glucose measurement units.

This screen shows the blood glucose measurement units (mg/dL or mmol/L).

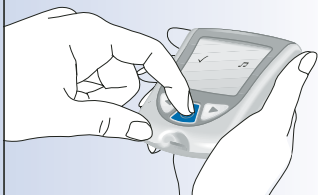

Press and release the **i** button to return to Set Beeper.

Press and Hold the ⓘ
button to turn your
monitor off.

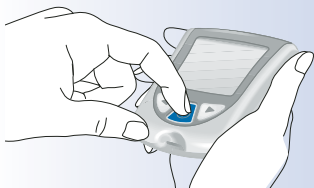

**You have successfully set
up your monitor.**

*Questions? Call
Customer Care:
1-800-527-3339*

CHAPTER 3

Calibrating Your Precision Xtra Monitor

► Why Calibrate Your Monitor?

Your Precision Xtra monitor must be calibrated so that it can recognize the test strip you are using. Calibration ensures that your results are accurate.

► When to Calibrate Your Monitor

- When you use the monitor for the first time.
- **EACH** time you open and use a new box of blood glucose or blood β -Ketone test strips.

Calibrating
Your Monitor

► What You Will Need


- Precision Xtra monitor
- For glucose calibration:
 - Blood glucose test strip
 - Blood glucose test strip instructions for use
 - Blood glucose test strip calibrator
- For β -Ketone calibration:
 - Blood β -Ketone test strip
 - Blood β -Ketone test strip instructions for use
 - Blood β -Ketone test strip calibrator

► How to Calibrate Your Monitor

When you insert a test strip for the first time, the display window shows:

This means the monitor is **not** calibrated for blood glucose monitoring.


This means the monitor is **not** calibrated for blood β -Ketone monitoring.

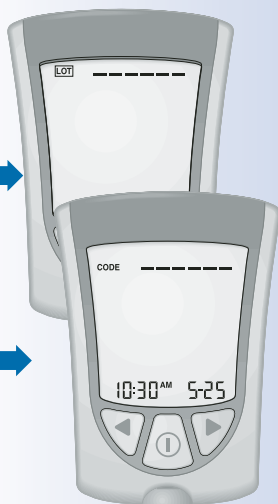

IMPORTANT:


- Use only the calibrator that is packaged in the box of test strips you are using.
- **Do not** use test strips that have expired. Check the expiration date on the test strip foil packet and test strip box. If only the year and month are shown, the expiration date is the last day of the month.

- 1 Remove the glucose or β -Ketone calibrator package from the new box of test strips.



- 2 Open the calibrator package. Find the three raised bumps on the calibrator package. Peel the clear cover away from the three raised bumps.

3 Hold the calibrator with the LOT number (glucose) or calibration CODE (β -Ketone) facing you.

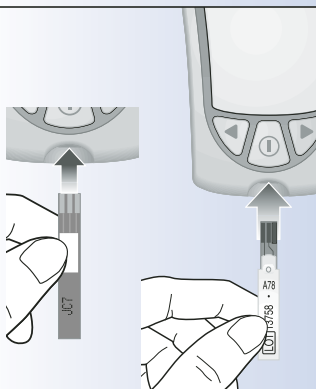

4 Insert the calibrator into the strip port. Push it in until it stops.

The Display Check shows on the display window, followed by the time, month, and day.

Next, the LOT number (glucose) or calibration CODE (β -Ketone) shows on the display window.

a. Example of glucose LOT number: **LOT 13758**

b. Example of β -Ketone calibration CODE: **CODE JC7**

Then you hear the beeper, if the beeper is ON.

Glucose



β -Ketone

5 Check that the LOT number or calibration CODE on all these items matches:

- ✓ Display window
- ✓ Test strip calibrator
- ✓ Test strip instructions for use
- ✓ Test strip foil packet

When the LOT number or calibration CODE on all these items matches:

What It Means:

Calibration is complete.

What to Do:

You may now monitor your blood glucose or blood β -Ketone.

When the LOT number or calibration CODE on all these items DOES NOT match:

What It Means:

Your monitor may not be calibrated for the box of test strips you are using.

What to Do:

- Check that you are using the calibrator that came in the box of test strips you are using.
- Try to calibrate again.

IMPORTANT: If the LOT number or calibration CODE still does not match, contact Customer Care. **Do not** attempt to monitor your blood glucose or blood β -Ketone. Your monitor may show an incorrect result.

6 Remove the calibrator from the monitor and store it in your monitor's carrying case.


IMPORTANT: Do not throw the calibrator away until you have used all of the test strips in the box.

If you have any trouble calibrating your system, please contact Customer Care.

► How to Recall the LOT Number or Calibration CODE


- 1 To recall the glucose LOT number, Press and Hold the ► button. While holding the ► button, Press and Hold the ⓘ button.

The Display Check shows on the display window, then the glucose LOT number shows with the time, month, and day of the most recent glucose calibration.



- 2 After the glucose LOT number is displayed, you can recall the β -Ketone calibration CODE. Press and Release the ► button or the ◀ button.

The β -Ketone calibration CODE shows with the time, month, and day of the most recent β -Ketone calibration.

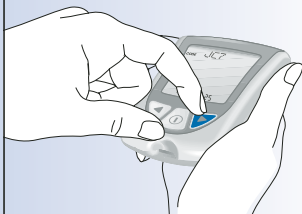

Note: If the LOT number or calibration CODE that shows on your monitor's display window is not correct:


What It Means:


Your monitor may not be calibrated for the box of test strips you are using.

What To Do:

- Re-calibrate your monitor.
- Check that you are using the calibrator that came in the box of test strips you are using.

Remember, improper calibration will cause incorrect results.

3 Press and Hold the  button to turn your monitor off.

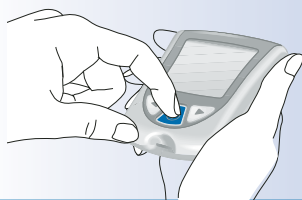

**Questions? Call
Customer Care:
1-800-527-3339**


Monitoring Your Blood Glucose

► What You Will Need

- Blood glucose test strip with its instructions for use
- Precision Xtra monitor calibrated to match the LOT number of the blood glucose test strip you are using
- Lancing device and a new, sterile lancet

► Important Information about Monitoring Your Blood Glucose

- **Do not** use out-of-date test strips. Check the expiration date printed on the test strip box and on each test strip foil packet. If only the month and year are printed on the test strip, then the expiration date is the last day of that month.
- For more detailed information about your test strip, please read its instructions for use before monitoring.
- Use the test strip **immediately** when you take it out of its foil packet.



Example:


**Expiration date
March 31, 2006**

- **Do not** use a wet, bent, scratched, or damaged test strip.
- **Do not** use the test strip if its foil packet has a puncture or tear in it.
- Before you monitor your blood glucose or blood β -Ketone, allow your monitor and test strip to reach the recommended operating range of the test strip. The test strip operating range is in the "Limitations of Procedure" section of your blood glucose test strip instructions for use.
- Read the lancing device instructions for use.

► How to Monitor Your Blood Glucose

Getting Started

- 1 Prepare your lancing device.



2 Wash your hands using warm soapy water and dry them completely.

3 Remove the test strip from its foil packet.

Note: For pictures that show how to open the blood glucose test strip foil packet, please see the information card in the box of blood glucose test strips.

Monitoring
Blood Glucose



4 Insert the three black lines at the end of the test strip into the strip port.



5 Push the test strip in until it stops.

The monitor turns on automatically.

These items show on the display window, one after the other:

- Display Check – Remember to make sure that all items in the picture here show on the display window. (See Chapter 1 for more information about the Display Check.)

- Time, month, and day (if set)

If date and time are not set, dashes will show instead of numbers.



- LOT number for the box of blood glucose test strips you are using.
-




- Apply Blood message, which tells you that the monitor is ready for you to apply blood to the blood glucose test strip.
-







Fingertip sampling

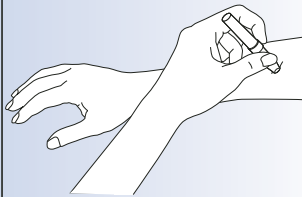

Forearm sampling



Upper arm sampling



Base of thumb sampling

Obtaining A Blood Drop

Use your lancing device to obtain a blood drop.

Recommendations for Obtaining a Blood Drop

- To obtain a sample from an alternative site (forearm, upper arm, or base of the thumb), use an appropriate alternative site lancing device.
- Before you obtain a blood sample from the fingertip, forearm, upper arm, or base of the thumb, make sure the sample site is clean, dry, and warm. To warm the sample site, wash it in warm water, rub the skin vigorously for a few seconds, or apply a warm pad to it.
- Hang your arm down before pricking your finger or the base of the thumb to help blood flow.
- To obtain a blood sample from the arm, use a fleshy area away from bone. Avoid areas where there is a lot of hair.
- Avoid squeezing the puncture site.
- Apply the blood sample to the test strip immediately.

Lancets and Lancing Device


- Lancets are for one-time use only. Use a new lancet each time you monitor.
- Discard your used lancet properly. Put it in an empty puncture-resistant container, such as a plastic milk carton or detergent bottle.
- Never share your lancing device or lancet with another person.

Applying the Blood Drop to the Test Strip

- 1 Touch the blood drop to the white area at the end of the test strip. The blood is drawn into the test strip.

Note: If the monitor shuts off before you apply blood to the test strip, remove the test strip from the monitor and try again.



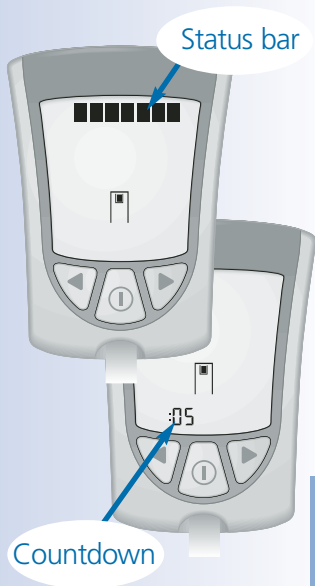

2 Continue to touch the blood drop to the end of the test strip until the monitor begins the test. The monitor begins the test when:

- You hear the beeper, if the beeper is ON.
- The display window shows the status bar.
- Then the display window shows the countdown.

Note: Do not remove the test strip from the monitor or disturb the test strip during the countdown.

Important: If the countdown does not start:

What It Means:

You might not have applied enough blood to the test strip.

What to Do:

- Apply a second drop of blood to the test strip. Refer to your test strip instructions for use for the number of seconds you have to apply a second drop.
- If the countdown still does not start, or if the number of seconds you have to apply a second drop have passed, discard the test strip, turn off your monitor, and try again with a new test strip.

Correct




Apply second drop



3 At the end of the countdown:

- If the beeper is ON, listen for the beeper.
- The blood glucose result shows on the display window.
- The result is stored in your monitor's memory. You may also write the result in your logbook.

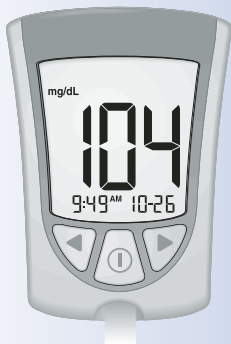


Shutting Off Your Monitor



- 1 Removing the test strip from the strip port turns off the monitor. You can use the opened foil packet to remove and discard your used test strip.

- 2 Discard the test strip properly.

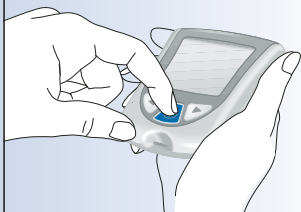

Note: You may also turn the monitor off by Pressing and Holding the ⓘ button. If you do not turn your monitor off or pull the test strip out, the monitor shuts off automatically after 60 seconds.

► Understanding Your Result


"LO" Result

What It Means:

Your monitor has determined that your blood glucose result is lower than 20 mg/dL (1.1 mmol/L) or there may be a problem with the test strip.

What to Do:

Monitor your blood glucose again with a new test strip. If **LO** shows on the display window again, contact your healthcare professional **immediately**.

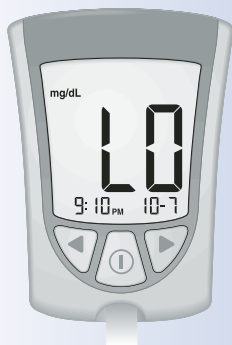


Result 300 mg/dL or Higher


When your blood glucose result is 300 mg/dL (16.7 mmol/L) or higher, **KETONES?** flashes on and off on the display window.

What to Do:

If you check your ketones as part of your diabetes management program, it is recommended that you check your blood β -Ketone.

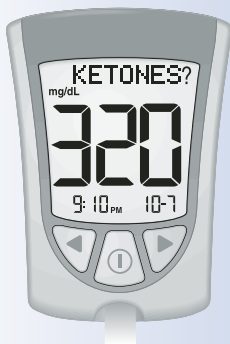

"HI" Result

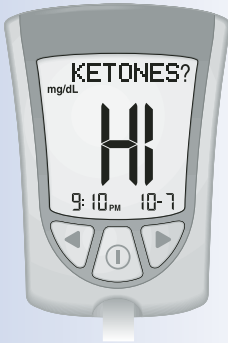

What It Means:

Your monitor has determined that your blood glucose result is higher than 500 mg/dL (27.8 mmol/L) or there may be a problem with the test strip.

What to Do:

Monitor your blood glucose again with a new test strip. If **HI** shows on the display window again, contact your healthcare professional **immediately**.

If you check your ketones as part of your diabetes management program, it is recommended that you check your blood β -Ketone.

Monitoring
Blood Glucose

"E-4" Result

What It Means:

Your blood glucose may be too high to be read by the system, or there may be a problem with the test strip.


What to Do:

Monitor your blood glucose again with a new test strip. If **E-4** shows on the display window again, contact your healthcare professional **immediately**.

Important:

It is recommended that you repeat the blood glucose test with a new test strip when:

- **LO** shows on the display window.
- You obtain a low blood glucose result, but you do not have symptoms of low blood glucose.
- Your monitor displays a blood glucose result that is unusually low, lower than 50 mg/dL (2.8 mmol/L).

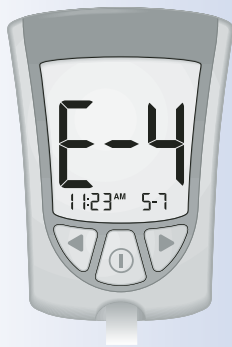

- **HI** shows on the display window.
- You obtain a high blood glucose result, but you do not have symptoms of high blood glucose.
- Your monitor displays a result that is unusually high, higher than 300 mg/dL (16.7 mmol/L).
- You question your result.

Important:

A result that is incorrect may have a serious medical outcome. Consult your healthcare professional before changing your diabetes medication program.

Monitoring Your Blood β -Ketone

*Questions? Call
Customer Care:
1-800-527-3339*

It is important to check your ketones when:

- You have an illness.
- Your blood glucose is higher than 300 mg/dL (16.7 mmol/L).
- You are experiencing unusual blood glucose results.
- You and your healthcare professional determine that it is necessary.

► What You Will Need

- Blood β -Ketone test strip with its instructions for use
- Precision Xtra monitor calibrated to match the calibration CODE of the blood β -Ketone test strip you are using
- Lancing device and a new, sterile lancet

► Important Information about Monitoring Your Blood β -Ketone

MediSense
β-Ketone Test Strip

Abbott Laboratories
Abbott Diabetes Care
Alameda, CA 94502
USA

LOT	70208
EXP	2006/03/09
CAL CODE	JC7
LO	0.3-0.7 mmol/l
MD	1.9-2.9 mmol/l
HI	3.7-5.7 mmol/l

Example:

Expiration date

March 9, 2006

- For more detailed information about your blood β -Ketone test strip, please refer to its instructions for use before monitoring.
- **Do not** use out-of-date test strips. Check the expiration date printed on the test strip box and on each test strip foil packet.
- **Do not** put urine on the blood β -Ketone test strip.
- Use the test strip immediately when you take it out of its foil packet.
- **Do not** use a wet, bent, scratched, or damaged test strip.
- **Do not** use the test strip if its foil packet has a puncture or tear in it.
- Use each test strip only once.
- Before you monitor your blood glucose or blood β -Ketone, allow your monitor and test strip to reach the recommended operating range of the test strip. The test strip operating range is in the "Limitations of Procedure" section of your blood β -Ketone test strip instructions for use.

Monitoring
Blood β -Ketone

- Monitoring
Blood β -Ketone
- Read the lancing device instructions for use.
 - The blood β -Ketone test strip foil packet contains a desiccant tablet (Zeolite - Sodium Calcium Aluminosilicate). Although this material is not considered dangerous¹, the following safety advice should be observed:

1. Keep away from children.
2. Do not expose to water as product gets hot and could cause burns.
3. Do not eat, and avoid contact with eyes and skin. May cause burns to the mouth and throat.
4. If swallowed, drink two glasses of water. Seek medical help.


► How to Monitor Your Blood β -Ketone

Getting Started

- 1 Prepare your lancing device.



2 Wash your hands using warm soapy water and dry them completely.

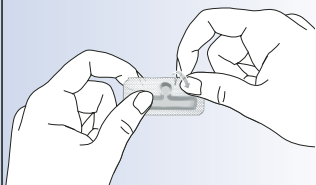

3 Remove the test strip from its foil packet.



4 Insert the three black lines at the end of the test strip into the strip port.



5 Push the test strip in until it stops.

The monitor turns on automatically.

These items show on the display window, one after the other:

- **Display Check** – Remember to make sure that all items in the picture here show on the display window. (See Chapter 1 for more information about the Display Check.)

- Time, month, and day (if set)

If date and time are not set, dashes will show instead of numbers.




- Calibration CODE for the box of blood β -Ketone test strips you are using.
-



- **KETONE** and Apply Blood message, which tell you that the monitor is ready for you to apply blood to the blood β -Ketone test strip.
-





Fingertip sampling

Obtaining A Blood Drop

Use your lancing device to obtain a blood drop.

Important: Blood β -Ketone test strips have not been evaluated for alternative site monitoring. **Use only fingertip blood samples for blood β -Ketone monitoring.**

Recommendations for Obtaining A Blood Drop

- Before you obtain a blood sample from the fingertip, make sure the sample site is clean, dry, and warm. To warm the sample site, wash it in warm water or rub the skin vigorously for a few seconds.
- Hang your arm down before pricking your fingertip to help blood flow.
- Avoid squeezing the fingertip.
- Apply the blood sample to the test strip immediately.


Lancets and Lancing Device

- Lancets are for one-time use only. Use a new lancet each time you monitor.
- Discard your used lancet properly. Put it in an empty puncture-resistant container, such as a plastic milk carton or detergent bottle.
- Never share your lancing device or lancet with another person.


Applying the Blood Drop to the Test Strip

- 1 Touch the blood drop to the purple area on the top of the test strip. The blood is drawn into the test strip.

Note: If the monitor shuts off before you apply blood to the test strip, remove the test strip from the monitor and try again.

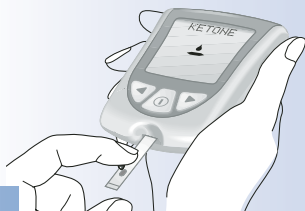

- 2 Continue to touch the blood drop to the purple area on the top of the test strip until the monitor begins the test. The monitor begins the test when:

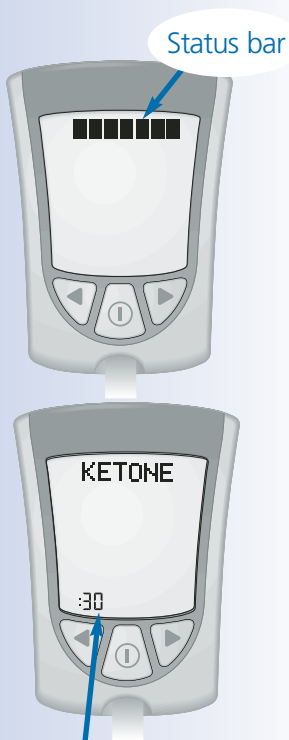

- You hear the beeper, if the beeper is ON.
- The display window shows the status bar.
- Then the display window shows the countdown.

Note: Do not remove the test strip from the monitor or disturb it during the countdown.

Important: If the countdown does not start:

What It Means:


You might not have applied enough blood to the test strip.

What to Do:

- Apply a second drop of blood to the test strip. Refer to your test strip instructions for use for the number of seconds you have to apply a second drop.
- If the countdown still does not start, or if the number of seconds you have to apply a second drop have passed, discard the test strip, turn off your monitor, and try again with a new test strip

3 At the end of the countdown:

- If the beeper is ON, listen for the beeper.
- The blood β -Ketone result shows on the display window with the word **KETONE**.
- The result is stored in your monitor's memory as a blood β -Ketone result. You may also write the result in your logbook.

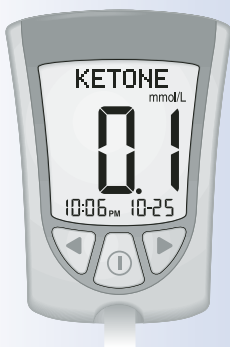


Shutting Off Your Monitor

- 1** Removing the test strip from the strip port turns off the monitor. You can use the opened foil packet to remove and discard your used test strip.



- 2** Discard the test strip properly.

Note: You may also turn the monitor off by Pressing and Holding the **(i)** button. If you do not turn your monitor off or pull the test strip out, the monitor shuts off automatically after 60 seconds.



► Understanding Your Result

Blood β -Ketone is expected to be lower than 0.6 mmol/L.³ Blood β -Ketone may be higher when a person is ill, is fasting, exercises vigorously, or if blood glucose levels are not controlled.²⁻⁴

When:

- Blood β -Ketone result is between 0.6 and 1.5 mmol/L and blood glucose result is 300 mg/dL (16.7 mmol/L) or higher:

What It Means:

A problem requiring medical assistance may be occurring.

What to Do:

Contact your healthcare professional. Follow his or her instructions for sick day management.

When:

- Blood β -Ketone result remains high or becomes higher than 1.5 mmol/L:

What It Means:

You may be at risk of developing diabetic ketoacidosis (DKA).³⁻⁷

What to Do:

Contact your healthcare professional **immediately**.


"HI" Result


What It Means:

Your monitor has determined that your blood β -Ketone result is higher than 6.0 mmol/L, or there may be a problem with the test strip.

What to Do:

Monitor your blood β -Ketone again with a new test strip. If **HI** shows on the display window again, contact your healthcare professional **immediately**.

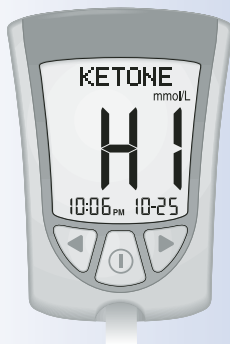

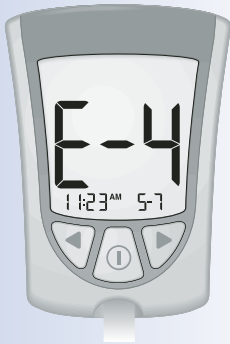

"E-4" Result

What It Means:

There may be a problem with the test strip.

What to Do:

Monitor your blood β -Ketone again with a new test strip. If **E-4** shows on the display window again, contact your healthcare professional **immediately**.

Important: It is recommended that you repeat the blood β -Ketone test with a new test strip when:

- **HI** appears in the display window.
- Your result is unusually high.
- You question your result.
- You obtain a 0.0 mmol/L blood β -Ketone result BUT your blood glucose is higher than 300 mg/dL (16.7 mmol/L).

Important: A result that is incorrect may have a serious medical outcome. Consult your healthcare professional before changing your diabetes medication program.

Doing A Control Solution Test

Questions? Call
Customer Care:
1-800-527-3339

► Why Do A Control Solution Test?

The control solution test tells you that your monitor and test strips are working correctly. A control solution test is similar to when you monitor your blood glucose or blood β -Ketone, except you use a MediSense Control Solution. **You do not use a drop of blood in a control solution test.**



► When Is Doing A Control Solution Test Recommended?

- When you question your results
- To make sure that your monitor and test strips are working properly

► Important Information about Control Solution Testing

- For more detailed information about control.

solutions, read the control solution instructions for use.

- MediSense Control Solutions may be used for glucose or ketone control solution testing.
- **Do not** use the control solution if the expiration date has passed. Check the expiration date printed on the control solution bottle.
- When you open a control solution bottle for the first time, count forward 90 days and write this date on the control solution bottle using a pen that won't smear or wipe off. Throw away any remaining solution after this date.
- The results obtained from control testing do not reflect your personal blood glucose or blood β -Ketone levels in any way.
- **Do not** swallow the control solution.
- **Do not** inject the control solution or use the control solution as eye drops.

► What You Will Need

- Precision Xtra monitor calibrated to match the LOT number (glucose) or calibration CODE (β -Ketone) of the test strip you are using
- Blood glucose or blood β -Ketone test strip and its instructions for use
- MediSense Control Solutions and instructions for use

► How to Do Control Solution Testing


Getting Started

- 1 Wash your hands using warm soapy water and dry them completely.



2 Remove the test strip from its foil packet.

Note: For pictures that show how to open the blood glucose test strip foil packet, please see the information card in the box of blood glucose test strips.

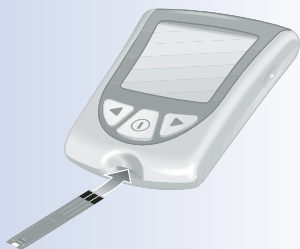

3 Insert the three black lines at the end of the test strip into the strip port.

4 Push the test strip in until it stops.

The monitor turns on automatically.

These items show on the display window, one after the other:

- Display Check – Remember to make sure that all items in the picture here show on the display window. (See Chapter 1 for more information about the Display Check.)



- Time, month, and day (if set)


If date and time are not set, dashes will show instead of numbers.





- LOT number (glucose) or calibration CODE (β -Ketone) for the box of test strips you are using.
- Apply Blood message, which tells you that the monitor is ready for you to apply control solution to the test strip.

Note: If you are doing a β -Ketone control solution test, **KETONE** will show on the monitor's display window with the β -Ketone Apply Blood message.

Control
Solution Testing



- 5** To mark the test as a control test, Press and Release the  button once.  shows on the display window.


Important: If you do not mark the test as a control test, it will be saved in your monitor's memory as one of your personal blood glucose or blood β -Ketone results. This could affect your blood glucose averages.

Applying Control Solution to the Test Strip

1 Turn the control solution bottle upside down three to four times to mix the solution.

2 Remove the cap.


3 Apply a drop of control solution to the test strip in the area shown here. The control solution is drawn into the test strip.



4 Continue to touch the control solution to the test strip until the monitor begins the test.

The monitor begins the test when:

- You hear the beeper, if the beeper is ON.
- The display window shows the status bar.
- Then the display window shows the countdown.

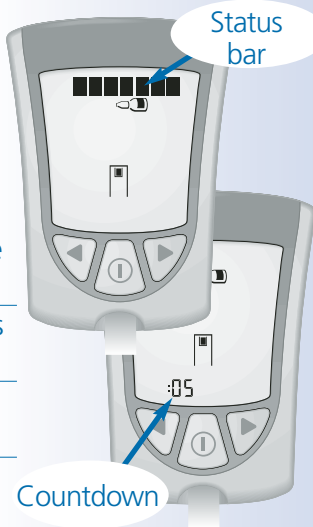

Note: Do not remove the test strip from the monitor or disturb it during the countdown.

Important: If the countdown does not start:


What It Means:

You might not have applied enough control solution to the test strip.

What to Do:

- Apply a second drop of control solution to the test strip. Refer to your test strip instructions for use for the number of seconds you have to apply a second drop.
- If the countdown still does not start, or if the number of seconds you have to apply a second drop have passed, discard the test strip, turn off your monitor, and try again with a new test strip.

Control
Solution Testing

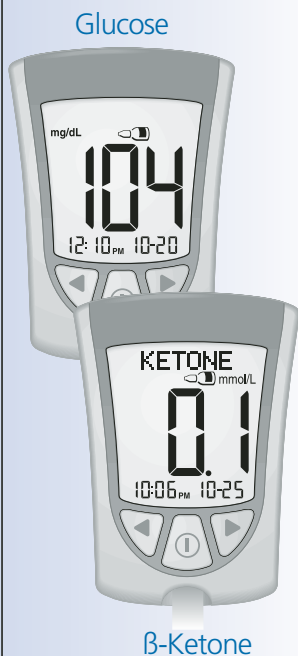

5 At the end of the countdown:

- If the beeper is ON, listen for the beeper.
- The control result shows on the display window.

Note: If you are doing a β -Ketone control solution test, **KETONE** will also show with the result.

- The result is stored in your monitor's memory as a control result. In your logbook, record the result as a control result.


Shutting Off Your Monitor

- 1 Removing the test strip from the strip port turns off the monitor. You can use the opened foil packet to remove and discard your used test strip.



- 2 Discard the test strip properly.

Note: You may also turn the monitor off by Pressing and Holding the **ⓘ** button. If you do not turn your monitor off or pull the test strip out, the monitor shuts off automatically after 60 seconds.



► Understanding Your Result

Compare the control result to the "Expected Results for Use with MediSense Control Solutions" range printed on:

- The blood glucose test strip instructions for use, for glucose control solution testing.
- The blood β -Ketone test strip instructions for use and foil packet, for β -Ketone control solution testing.

If the control result falls within the range:

What It Means:

Your monitor and test strips are working correctly.

If the control result does not fall within the range:

What It Means:

Your monitor and test strips may not be working correctly.

What to Do:

Repeat the test with a new test strip and ensure the control solution testing instructions are followed completely. If the result is still not within the printed range, contact Customer Care.

Reviewing & Using Your Results

Questions? Call
Customer Care:
1-800-527-3339

► What Can Your Monitor Show You?

Memory

Your Precision Xtra monitor has a memory that stores up to 450 events. This is a combination of control results, your personal blood glucose and blood β -Ketone results, and other monitor information.

You can review up to 450 of your most recent events on your monitor's display window.

Glucose Averages

You can view the average of all your blood glucose results from the last 7, 14, or 30 days. If you marked your control solution tests, the averages do not include control solution results. (For more information on marking control solution tests, see Chapter 6.)



Important:

- To review blood glucose averages, you **must** set the date and time before monitoring.
- If you **do not** mark control solution tests, this may affect your glucose averages.
- Blood glucose averages **do not** include blood β -Ketone results, glucose control results, β -Ketone control results, or results that do not show the time, month, and day.
- When there are no previous results or blood glucose averages to review, the display window shows three dashes.



► How to See Results in Memory

- 1 Begin with your monitor turned off. Make sure there is nothing in the strip port.

2 Press and Release the  button.

- The Display Check shows on the display window.
- Then your most recent result shows with its units on the monitor's display window, along with the time, month, and day that you got the result. (To set the correct date and time, follow the steps in Chapter 2.)

A blood glucose result in Memory will show with the letters **MEM**.

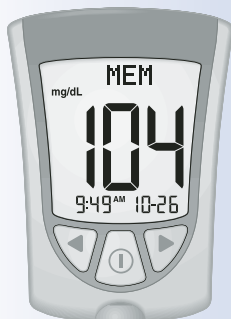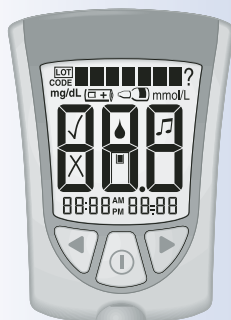


Blood Glucose result in Memory

A blood β -Ketone result in Memory will show with the letters **KET MEM**.



Blood β -Ketone result in Memory

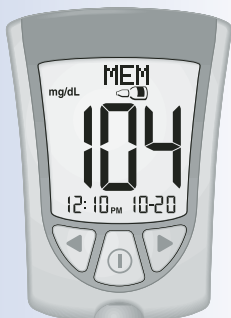


Glucose control solution result in Memory



β -Ketone control solution result in Memory

A control solution result in Memory shows with a control bottle, as long as you marked the test as a control solution test.

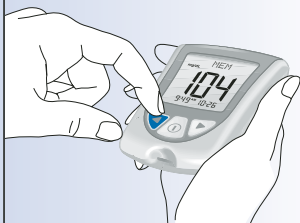


3 To review previous results, Press and Release the ◀ button once per result.

4 When you reach the last result in Memory, the display window shows three dashes.



5 To return to a result you previously reviewed, Press and Release the ► button once per result.



► How to See Averages


Important:

- Results that show as **LO** during blood glucose monitoring are included as 20 mg/dL (1.1 mmol/L) in blood glucose averages.
- Results that show as **HI** during blood glucose monitoring are included as 500 mg/dL (27.8 mmol/L) in blood glucose averages.




- 1 While in Memory, Press and Release the **1** button at any time to see the 7-Day average of your blood glucose results.


Note: n means how many tests were performed within the 7-, 14-, or 30-Day average period.



- 2 Press and Release the **◀** button once to see the 14-Day average of your blood glucose results.



- 3 Press and Release the **◀** button again to see the 30-Day average of your blood glucose results. If you Press and Release the **◀** button again, the display window shows the 7-Day average.




- 4 Press and Release the **1** button at any time to return to Memory.

5 Press and Hold the ⓘ button to turn off your monitor. Otherwise, the monitor turns off after 30 seconds.



► Transferring Your Results to a Computer

The results in your Precision Xtra monitor's memory, along with the time and date of the reading, can be transferred to a computer with the use of the Precision Link® Direct Software Version 2.5 and a Precision Link communications cable. For information on how to purchase the software and cable, contact Customer Care at 1-800-527-3339. To install the software, please follow the instructions provided in the Precision Link User's Guide.

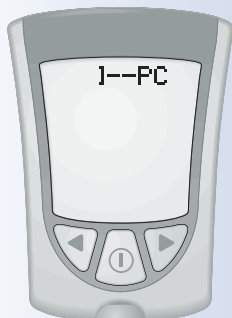

**Questions? Call
Customer Care:
1-800-527-3339**

Understanding & Troubleshooting Error Messages


There are times when error messages may show on your monitor's display window.

In the next few pages, we describe the error messages that may show on your monitor's display window, what they mean, and what you need to do.

Message

What It Means

What You Need to Do

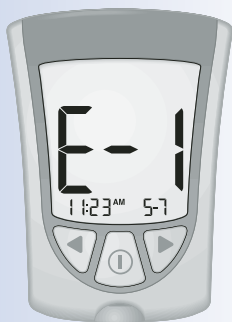

Temperature is too hot or too cold for the system to work properly.

- **Move your monitor and test strips to a location where the temperature is appropriate and monitor again with a new test strip. You may have to wait for your monitor to adjust to the new temperature. Refer to your test strip instructions for use for the appropriate operating range.**
- **If the error message appears again, contact Customer Care.**

What It Means

What You Need to Do

Message

Monitor error.

- Turn the monitor off, then repeat previous monitoring steps.
- If the error message appears again, contact Customer Care.



There may be a problem with the test strip.


- Review the monitoring instructions.
- Monitor again with a new test strip.
- If the error message appears again, contact Customer Care.



Message

What It Means

What You Need to Do

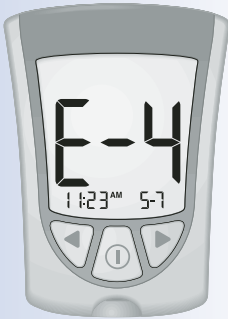


Blood glucose result may be too high to be read by the system.

OR

There may be a problem with the blood glucose or blood β -Ketone test strip.

- **Monitor again with a new test strip.**
- **If the error message appears again, contact your healthcare professional immediately.**

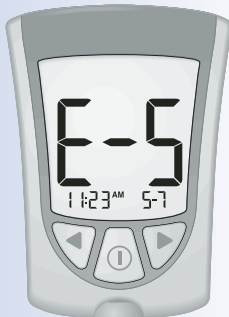

Blood applied to test strip too soon.

- **Review the monitoring instructions.**
- **Monitor again with a new test strip.**
- **If the error message appears again, contact Customer Care.**


What It Means

Calibration/Test strip error.

What You Need to Do

- Repeat the calibration using the calibrator bar that came with the test strip you are using.
- Check the date setting on your monitor.
- Check the expiration date on the test strip foil packet.
- If the error message appears again, contact Customer Care.

Message

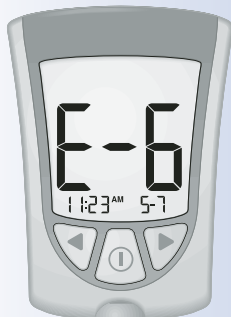

Test strip error.

Test strip is damaged, used, or the monitor does not recognize it.


- Monitor again using a test strip designed for use with Precision Xtra.
- If the error message appears again, contact Customer Care.



Message

What It Means

What You Need to Do

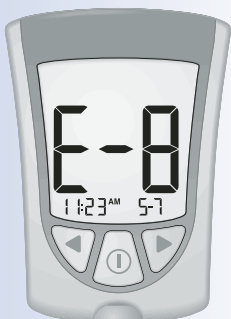

Monitor error.

- Remove test strip, turn monitor off, and try to monitor again.
- If the error message appears again, contact Customer Care.



Monitor error.

- Remove test strip, turn monitor off, and try to monitor again.
- If the error message appears again, contact Customer Care.

Your Monitor's Specifications & Limitations

Questions? Call
Customer Care:
1-800-527-3339



Size

Length 2.94" (7.47 cm)

Width

Top 2.10" (5.33 cm)

Bottom 1.70" (4.32 cm)

Thickness 0.64" (1.63 cm)

Weight

1.48 ounces (42 grams)

Power Source

One CR 2032 Lithium (coin cell) battery

Battery Life

Approximately 1,000 tests

Memory

Up to 450 events including control results, personal blood glucose and blood β -Ketone results, and other monitor information.

Storage Temperature

Monitor:	-13° to 131°F (-25° to 55°C)
Test Strips:	See test strip instructions for use.
Control Solution:	See control solution instructions for use.

Blood Glucose Assay Range

See blood glucose test strip instructions for use.

Blood β -Ketone Assay Range

See blood β -Ketone test strip instructions for use.

Control Solution Range

See blood glucose or blood β -Ketone test strip instructions for use.

Functions

- Blood glucose monitoring
- Blood β -Ketone monitoring
- Memory
- Glucose averaging: 7-Day, 14-Day, and 30-Day Averages
- Control solution marking and testing
- Backlight: If ON – Stays ON during countdown; turns OFF 30 seconds after result is displayed. If OFF – Stays OFF during countdown; stays OFF during data upload.
- Beeper: If ON – Beeps when calibrator is fully inserted and when countdown starts and finishes.

Data port Yes

Monitor Operating Range

Temperature: 50° to 122°F (10° to 50°C)

Relative Humidity: 10% to 90%, non-condensing

System Operating Range

Temperature: The system operating range is the operating range of the test strip you are using. See “Limitations of Procedure” section in test strip instructions for use.

Relative Humidity: 10% to 90%, non-condensing



Important Information about Using Blood Samples from the Forearm, Upper Arm, or Base of the Thumb:

- Contact your healthcare professional before you begin using any one of these alternative sites to test your blood glucose.
- Sampling from any one of these alternative sites may cause minor bruising and may leave marks that go away in a short time.
- There may be times when alternative site results are different from fingertip results. This happens when blood glucose levels change rapidly (for example, after you eat a meal, after you take insulin, or during or after exercise).
- Use alternative sites to monitor your blood glucose before, or more than two hours after, you eat a meal, take insulin, or exercise.

• **Do not** use blood samples from alternative sites when:

1. You think your blood glucose is low or is changing rapidly,
2. You have been diagnosed with hypoglycemic unawareness,
3. The results from alternative sites do not match the way you feel,
4. It is within two hours of eating a meal, taking insulin, or exercising, or
5. You monitor your blood β -Ketone.

*Questions? Call
Customer Care:
1-800-527-3339*

Caring For Your Monitor

► Cleaning Your Monitor

Store your monitor in its carrying case.

If the surface of your monitor gets dirty, you may clean it. Use a damp cloth and mild soap.

Healthcare professionals:
Acceptable cleaning solutions include 10% Bleach, 70% Alcohol, or 10% Ammonia.

Important:

Do not try to clean the strip port.


Do not pour liquid into the strip port or buttons.

Do not place your monitor in water or any other bath.


► Replacing Your Monitor's Battery

When your monitor needs its batteries replaced, the display window shows one of two things:

This means the battery is low. You may still use your monitor and the results will be accurate. However, the backlight is not useable. It is recommended that you replace the battery at this time.

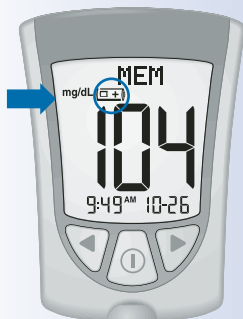

This means the battery must be replaced. The monitor is not useable. The monitor turns off automatically.

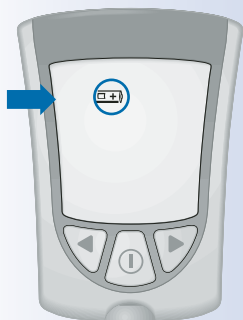


Important:

Do not remove the old battery until you have a new battery to install. It may be necessary to reset the time and date once you install a new battery.


How to Replace Your Monitor's Battery



- 1 Gently push the battery cover in and up with your thumb.




- 2 Lift the battery cover out of the monitor.




- 3 Pull on the plastic tab sticking out of the monitor to remove the old battery.


- 4 Insert a new CR 2032 Lithium (coin cell) battery with the plus sign (+) facing up.

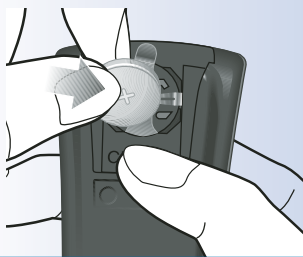


- 5 Place the notches on the battery cover into the appropriate molded areas.

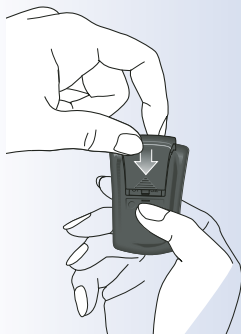

- 6 Gently push the battery cover in and down until you hear a click.

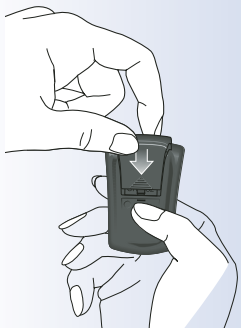



7 Press and Hold the ① button to turn your monitor on. If your monitor does not turn on, review the battery installation steps and reinstall the battery.

8 Check the date and time on your monitor. You may need to reset the date and time. (See Chapter 2, Setting Up Your System).

9 Be sure to discard the old battery in compliance with your local government's regulations.

Support, Guarantee & Limited Warranty

*Questions? Call
Customer Care:
1-800-527-3339*

▶ Support

Abbott Laboratories, Abbott Diabetes Care, is committed to providing you with support. Call us with any questions you may have about your Precision Xtra monitor:
1-800-527-3339.

Outside the United States, please contact your local Abbott Laboratories, Abbott Diabetes Care office or distributor.

You can view interactive product demonstrations online at: AbbottDiabetesCare.com

► Guarantee & Limited Warranty

Precision Xtra Advanced Diabetes Management System:

Abbott Laboratories Inc., Abbott Diabetes Care (“Abbott”) offers a Limited Warranty, as set forth below, to consumers who buy a Precision Xtra Advanced Diabetes Management System (“Monitor”) within the United States. Other purchasers, please contact your local authorized Abbott distributor for information about possible guarantee and/or warranty coverage for your purchase.

90-day Guarantee: Abbott offers consumer purchasers a 90-day money back guarantee. If you are not fully satisfied with your Monitor, call Customer Care at 1-800-300-0978 (toll free) for a full refund. Refund will be limited to amount paid by consumer net of any rebates. You must have a copy of the dated itemized purchase receipt and the original packaging to obtain this refund.

Limited Warranty: Under the standard warranty your new Monitor is covered for a period of four years from the original date of purchase, as long as it has not been modified, altered, or misused. **Lifetime Warranty is a benefit of enrollment in the Precision Friends for Life Program** and choice of replacement monitor will be at the discretion of Abbott.

Under the warranty, Abbott will replace, free of charge, this Monitor, if it is defective in material or workmanship. NO OTHER WARRANTIES, EXPRESS OR IMPLIED, ARE MADE. ABBOTT WILL NOT BE LIABLE FOR ANY INCIDENTAL OR CONSEQUENTIAL DAMAGES RESULTING DIRECTLY OR INDIRECTLY FROM THE FAILURE OF THE PRODUCT TO PERFORM IN ACCORDANCE WITH SPECIFICATIONS.

Some states do not allow the exclusion or limitation of other express or implied warranties or incidental or consequential damages, so the above limitations or exclusions may not apply to you.

For Warranty Service, contact Customer Care for assistance and/or instructions for obtaining a replacement monitor at 1-800-527-3339. Abbott may require, as a condition to obtaining warranty service, that you return the Monitor, postage prepaid, to an address specified by Customer Care.

Your Rights Under State Law: This warranty gives you specific legal rights, and you may also have other rights that vary from state to state.

Free Lifetime Monitor Upgrades: Monitor upgrade requires enrollment in the Precision Friends for Life Program and use of your Monitor for a minimum of three years. Choice of replacement monitor will be at the discretion of Abbott.

References

1. Directive 1999/45/EC of the European Parliament and of the Council of 31 May 1999 concerning the approximation of the laws, regulations and administrative provisions of the Member States relating to the classification, packaging and labelling of dangerous preparations.
2. Schade DS, Eaton RP. Metabolic and clinical significance of ketosis. *Special Topics in Endocrinology and Metabolism* 1982; 4:1–27.
3. Wiggam MI, O’Kane MJ, Harper R, Atkinson AB, Hadden DR, Trimble ER, Bell PM. Treatment of diabetic ketoacidosis using normalization of blood 3-hydroxybutyrate concentration as the endpoint of emergency management. *Diabetes Care* 1997; 20:1347–52.
4. Harano Y, Kosugi K, Hyosu T, Suzuki M, Hidaka H, Kashiwagi A, Uno S, Shigeta Y. Ketone bodies as markers for Type 1 (insulin-dependent) diabetes and their value in the monitoring of diabetes control. *Diabetologia* 1984; 26:343–8.
5. Ubukata E. Diurnal variation of blood ketone bodies in insulin-dependent diabetes mellitus and non-insulin-dependent diabetes mellitus patients: The relationship to serum C-peptide immunoreactivity and free insulin. *Ann Nutr Metab* 1990; 34:333–42.
6. Luzi L, Barrett EJ, Groop LC, Ferrannini E, DeFronzo RA. Metabolic effects of low-dose insulin therapy on glucose metabolism in diabetic ketoacidosis. *Diabetes* 1988; 37:1470–77.
7. Hale PJ, Crase J, Nattrass M. Metabolic effects of bicarbonate in the treatment of diabetic ketoacidosis. *Br Med J* 1984; 289; 1035–8.

Distributed by:
Abbott Laboratories
Abbott Diabetes Care
Alameda, CA 94502
USA

Customer Care available 24 hours a day, 7 days a week at 1-800-527-3339
or visit us online at: AbbottDiabetesCare.com

Reorder No.: 70297-01

MediSense and Precision Xtra are trademarks of Abbott Laboratories.

© 2005 Abbott Laboratories.



PRT06986 Rev. B 8/05

ART06986 Rev. B 8/05